


EM=480


LCMS Scan ESI+

Ret. Time: 1.66

<<<< NEGATIVE SPECTRA >>>>

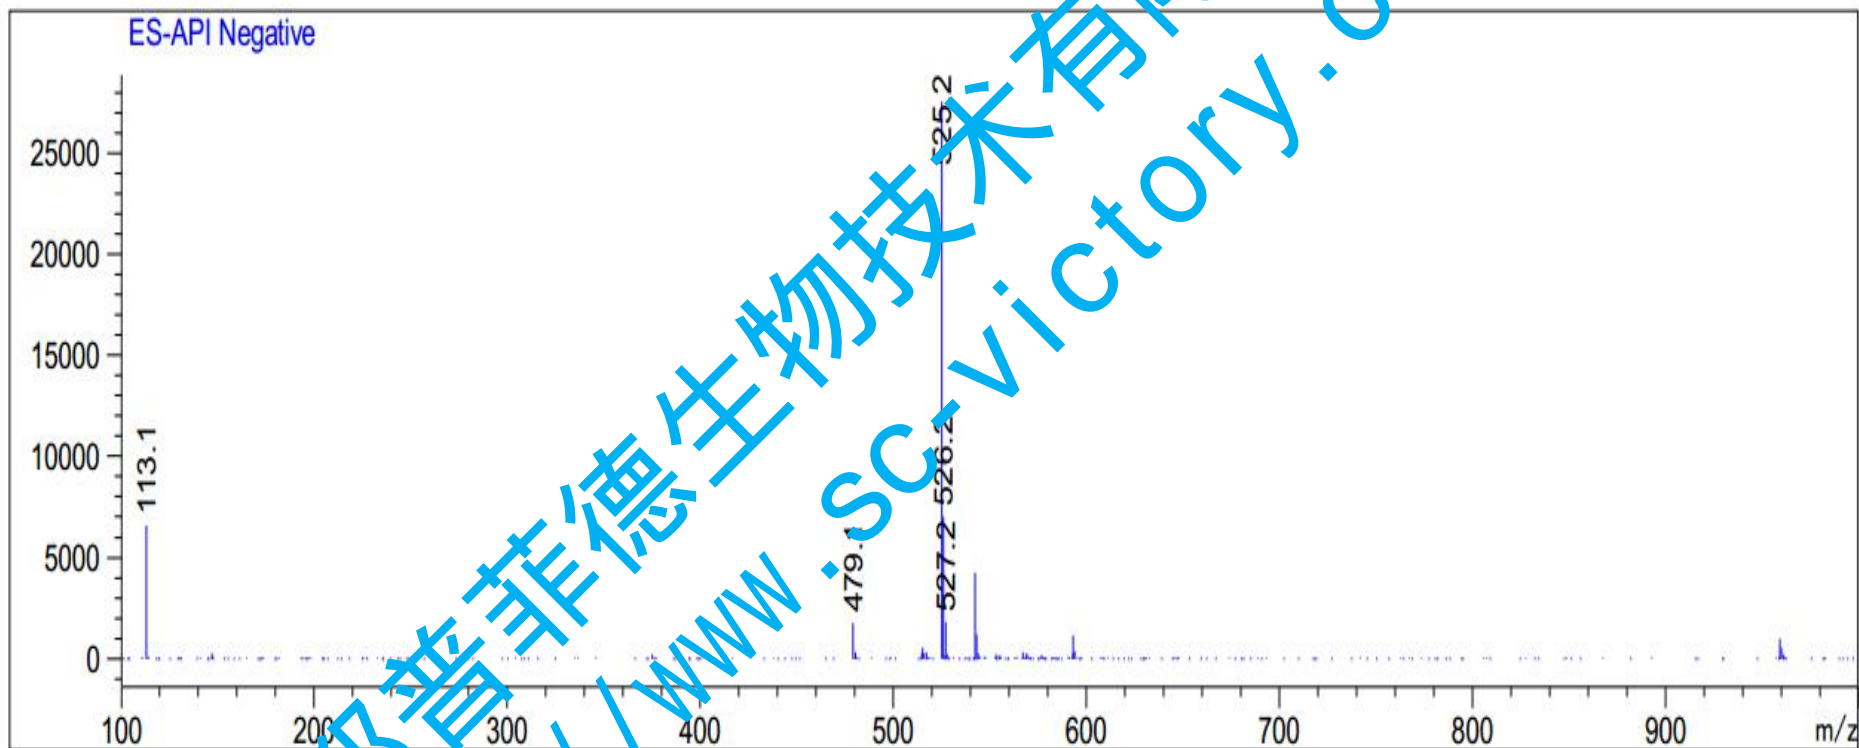

Ret. Time: 2.73

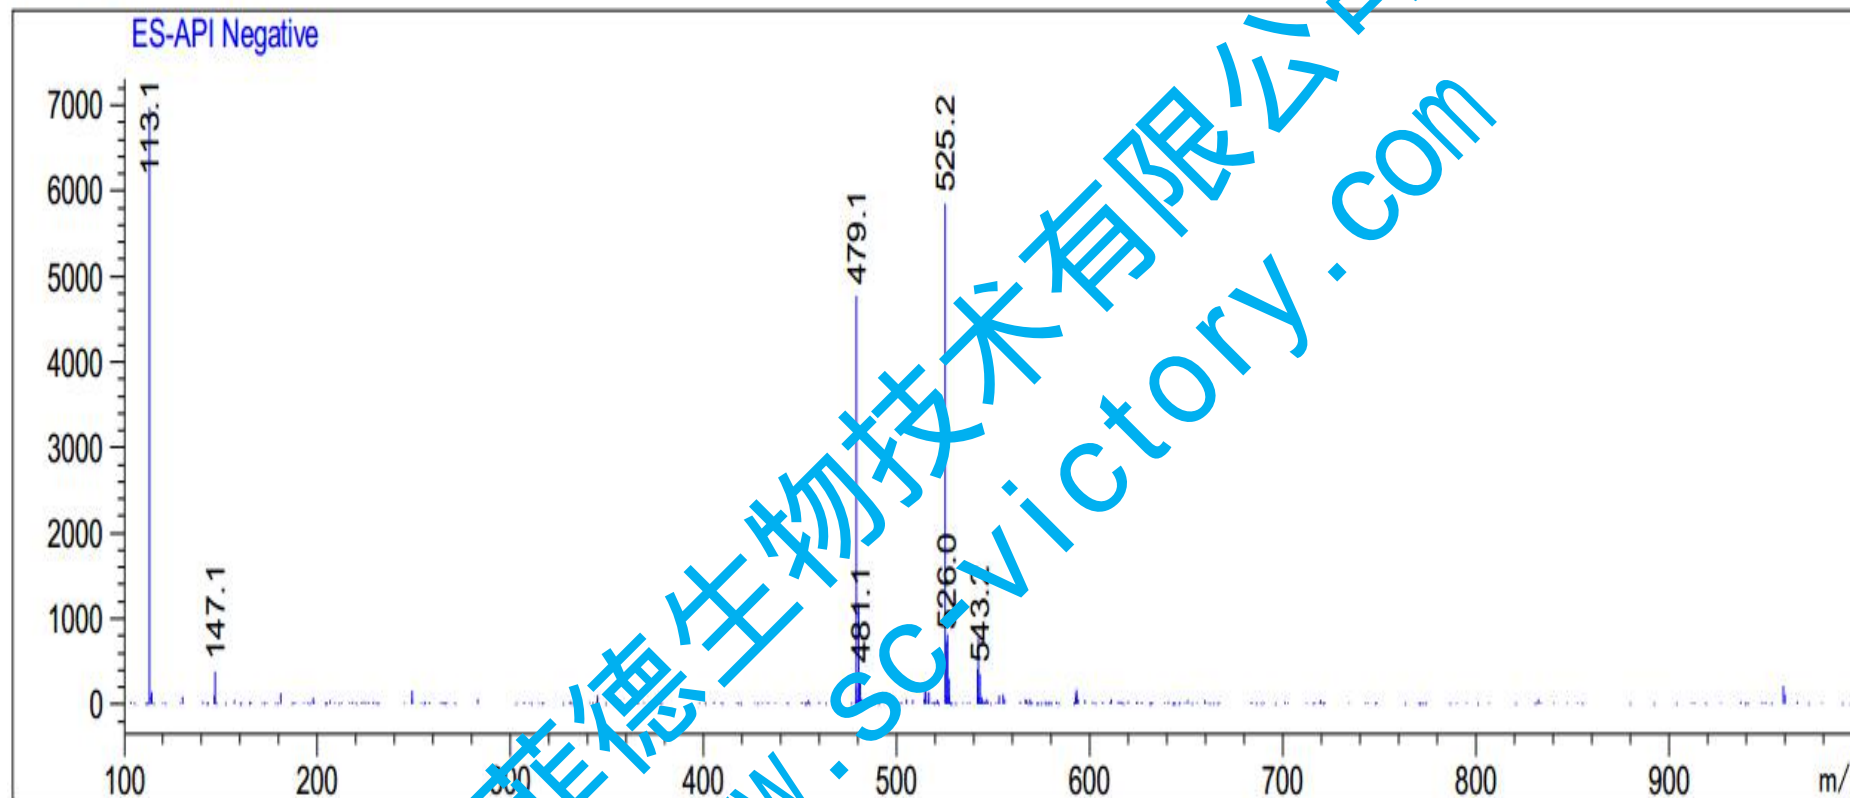

成都普菲德生物技术有限公司
<http://www.sc.victory.com>